

United Nations Population Fund, UNFPA 131, 31 August 1989 street, Chisinau, Republic of Moldova, MD-2012

Fiscal Code: 12626016 Tel: +373 79785684 Website: www.unfpa.org

Date: <u>06/06/2023</u>

Request for Quotation No. UNFPA/MD/RFQ/017/2023

Dear Sir/Madam,

We hereby solicit your quotation for the supply of Medical Supplies and Consumables named below to UNFPA warehouse at CPT Incoterms:

UNFPA warehouse:

Vitra Building

Str. Industriala 5

Chisinau, Republic of Moldova,

Google map link:

https://goo.gl/maps/nVN19BpARyve8Myy6

#	Description of goods / services: Generic technical specifications for goods / ToR for services	Unit of measure	Quantity
	UNFPA Equipment		
	Waxed block Archive		
	General Description: Medical furniture used for long-term storage of the examined lamellae Intendent of use: It is used in morpho pathological laboratories for long-term waxed block storage Product Description: Location mode on the floor; stainless steel, corrosion protected; Modular cabinet type with drawers.		
1	 General description: Storage space: Cabinet dimensions About 110 x 60 x 70 cm, possibility to stack one above the other Number of blocks stored in one cabinet - minimum 20 000 The dimensions of every waxed block 30 mm x 40 mm. The position of the waxed block vertical; 	Units	20
	Accessories, Consumables, Spare parts, and Other Components: • Shelf divider for blocks Documentation and Requirements: • Instructions for use and service manuals to be provided (including procedures for decontamination) • User language preference prioritized; English is mandatory. • Contact details of manufacturer, supplier and local service agent.		



- Certificate of calibration and inspection to be provided (if applicable).
- List to be provided of equipment and procedures required for local calibration and routine maintenance.
- List to be provided of common spares and accessories, with part numbers.

Regulatory & Conformity Requirements:

- CE mark conforming to Medical Device Regulation 2017/745 or 93/42
- Manufacturer's Quality Management System is certified to ISO 13485
- Manufacturer's Quality Management System is certified to ISO 9001

Safety & Product Standards:

- Standards ISO 9001, ISO 13485;
- Compliant with active version of the following standards (or equivalent):

General manufacturing:

- ISO 13485: Medical Devices Quality Management Systems -Requirements for Regulatory Purposes
- ISO 14971: Medical Devices Application of Risk Management to Medical Devices
- ISO 15223-1: Medical devices -- Symbols to be used with medical device labels, labelling and information to be supplied -- Part 1: General requirements
- IEC 60601-1 Medical electrical equipment Part 1: General requirements for basic safety and essential performance

Installation Requirements:

• Device should be installed at required place

Training Requirements:

• Training of users in operation and basic maintenance shall be provided.

Environmental Conditions:

- Environmental conditions vary globally and can be extreme; however, the following are tenable:
- Operating temperature: 15°C to 35°C
- Operating relative humidity: ≤ 85%, non-condensing
- It is the responsibility of the procurement body to ensure that
 the manufacturer's recommended operation and storage
 conditions are respected. If the device requires that the
 operating and/or storage environment be climate-controlled,
 appropriate temperature and humidity control systems, including
 monitoring, should be applied to avoid premature material
 disintegration and/or device failure.

Estimated Life Span:

10 years

Warranty:

Minimum 5 years




	Specific inclusions and exclusions to be listed. Contact details of		
	manufacturer, supplier and local service agent to be provided. Centrifuge, for blood bank (10-12 tubes) low speed		
2	Description Laboratory centrifuges are intended to centrifuge blood. Rotational speed from 1000 to 4500 rpm Tubes of 10 - 15 ml Number of tubes 10-12 tubes Time range of work 0 - ≥60 min Step of incrementing of time ≤1 min Security Locking the cover during work yes Indicators Visual and acoustic indicators for Unbalance yes and Open cover yes Display Digital yes Noise level ≤70 dB Window, hole or other access, necessary to perform the periodical verification procedure yes Device must to have CE certificate for medical devices Yes Device guarantee minimum 2 years	Units	19
3	Centrifuge, (22 – 26 capillaries), for laboratory for hematocrit determination Description Laboratory centrifuges are intended to centrifuge blood for blood cells sedimentation and hematocrit determination. Rotational speed from 200 to 13000 rpm Compatible capillaries 1,6 mm external diameter, length 75 mm Number of capillaries 20 – 26 capillaries Time range of work 0 - ≥90 min Step of incrementing of time ≤1 min, Continuous operation Security Locking the cover during work yes Indicators Visual and acoustic indicators for Unbalance yes and Open cover yes Display Digital yes Noise level ≤65 dB Window, hole or other access, necessary to perform the periodical verification procedure yes Device must to have CE certificate for medical devices Yes Device guarantee minimum 2 years	Units	5
4	Z-fold thermal paper Z-fold thermal paper compatible with Fazzini FM5000C with 130 - 150 pages.	Package	570



	On paper must be drawn: The grid for the contractions pressure with		
	interval from 0 to 100 mmHg also indicated in kPa, with height of the grid		
	of 40 mm, and start at 10 mm from the bottom of the paper sheet;		
	The grid for the new born heart rate with interval from 30 to 240 BPM,		
	with height of the grid of 70 mm, and start at 64 mm from the bottom of		
	the paper sheet.		
	Paramedical case (box) with adjustable separators		
5	Multi-use, adaptable spaces, without content, housing resistant to mechanical actions, chemicals, disinfectants, (aluminium or polymers). Removable trays are easy to wipe down to keep sanitized. Storage bracket keeps used and sharp objects contained. Adustable separators should provide at least 8 separated spaces LxWxH: (at least) 400 mm x 300mm x 100 mm	25	Units



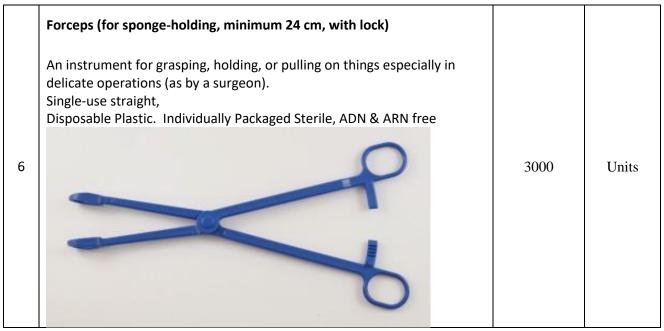

The goods are to be delivered maximum in **90 calendar days** upon issuing of PO. The quotation shall be valid at least for 90 days after the RFQ closing date.

Note: Partial bids will be accepted.

If you are interested in submitting a quotation for these items, kindly fill in the attached Quotation Form and send by email to the address indicated below:

Email: tender.mda@unfpa.org

Please submit your quotation in **MDL** (**local suppliers**) or **USD** (**international suppliers**) currency. Conversion of currency into the UNFPA preferred currency, if the offer is quoted differently from what is required, shall be based only on <u>UN Operational Exchange Rate</u> (https://treasury.un.org/operationalrates/OperationalRates.php) at the competition deadline date.

Your earliest response to this query would be highly appreciated, but not later than 13/06/2023, 16:30 (GMT +3, Moldova Local Time).

Note: Current UNFPA supplier policies apply to this solicitation and can be found at: http://www.unfpa.org/suppliers.

Qualification Criteria:

- Full acceptance of the PO/Contract General Terms and Conditions
- Maximum delivery period not to exceed 90 calendar days upon issuing of PO.
- Provided quotation with catalogue or detailed technical description including picture of each item quoted for.
- Written Self-Declaration of not being included in the UN Security Council 1267/1989 list, UN Procurement Division List or other UN Ineligibility List;
- Filled Fast Track Procurement Questionnaire for Medical Devices
- Regulatory and quality requirements for the manufacturer (ISO 13485, ISO 9001, preferable ISO14001)

Page 5 of 8



Evaluation method:

• Lowest priced offer that is substantially responsive to the requirements of the RFQ

Conditions for Release of Payment:

- Passing Inspection
- Written Acceptance of Goods based on full compliance with RFQ requirements

Best regards,

DocuSigned by:

Ivrie Tarcenco Prepared by: -85CA7739315F46C..

Tarcenco Iurie/ Procurement Analyst

Tel. No. +373 79785684

Email: tarcenco@unfpa.org

Approved by:

Mgina Ibaszade —43D750472CF14D1... Nigina Abaszade

Resident Representative

DocuSigned by:

UNFPA Moldova



Quotation Form

Name of Bidder:	
Date of Bid:	
Request for Quotation No:	
Currency of Bid price:	
Delivery time (from receipt of order till dispatch):	
Expiration of Validity of Quotation (The quotation shall be valid for a period of at least	90 days after
the Closing date.)	
Duice Calcadula.	

Price Schedule:

No.	Item	Quantity	Unit Price (Insert Currency)	Total CPT, Chisinau (Currency)	Delivery schedule
1	Waxed block Archive	20			
2	Centrifuge, for blood bank (10-12 tubes) low speed	19			(days)
3	Centrifuge, (22 – 26 capillaries), for laboratory for hematocrit determination	5			(days)
4	Z-fold thermal paper	570			(days)
5	Paramedical case (box)	25			(days)
6	Forceps (for sponge- holding, minimum 24 cm, with lock)	3000			(days)

In your offer, please include the following (mandatory documents):

- 1. Detailed technical description of the offered goods, or product catalogue/leaflet, with detailed technical specifications as detailed in RFQ. Photos of the device product and packaging (preferably in a format where the dimensions and features can be visually verified)
- 2. Quality standard of the products (Quality Certificates (ISO, EC etc.)):
- 3. Company registration documents
- 4. Written Self-Declaration of not being included in the UN Security Council 1267/1989 list, UN Procurement Division List or other UN Ineligibility List;
- 5. Fast Track Procurement Questionnaire for Medical Devices

Vendor's Comments:		
rentor's comments.		



I hereby certify that this company, which I am duly	authorized to sign for, accepts the terms and
conditions of UNFPA (http://www.unfpa.org/resou	urces/unfpa-general-conditions-contract) and
we will abide by this quotation until it expires.	
	D
Name and title	Date and Place